




ONE-HANDED OPERATION INSTRUCTIONS

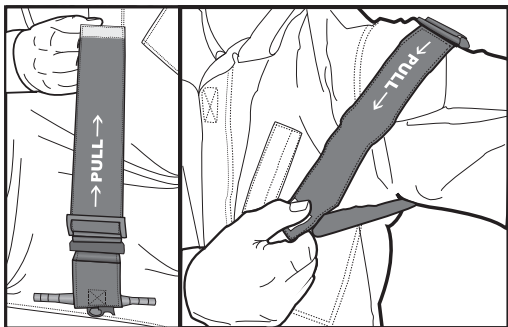


1 Hold the end of the strap by the white time label tab, allow the TMT to fall open with the word "PULL" facing away from you. Place around the injured extremity high and tight above the wound.

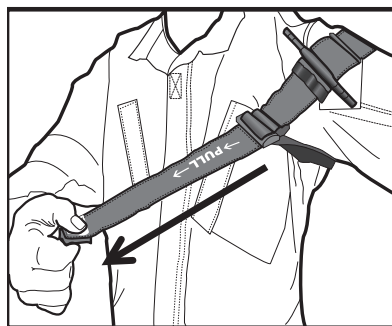


2 Pull time tab until Velcro® Brand material tail is separated from the TMT.

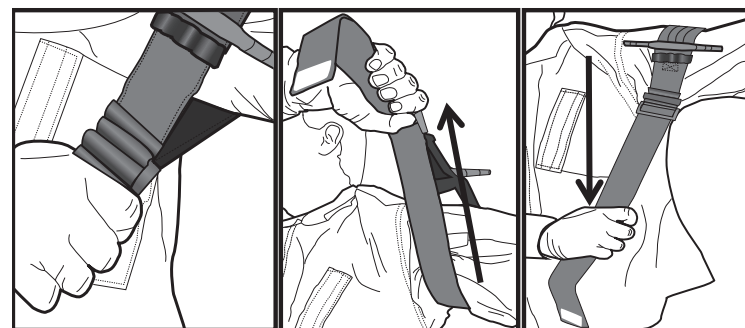


3 Grip tail close to the buckle, firmly pull up, out and away from the body and then downward in a quick ratcheting motion. Repeat step until snug around extremity.

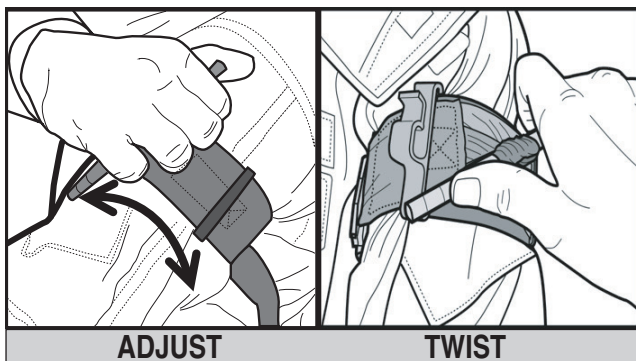

4 Adjust/rotate the TMT on extremity for ease of access to the torsion bar. Twist torsion bar until bleeding stops and the pulse is not present.

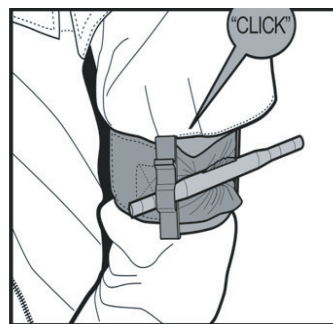

5 Lock the torsion bar into the retainer. Secure excess strap with Velcro® Brand material.

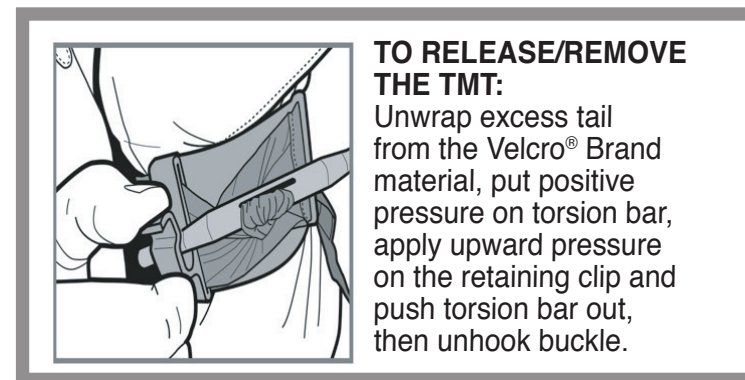

REMOVAL



Distributed by:
Combat Medical
5555 Harrisburg Industrial Park Drive
Harrisburg, NC 28075 USA
1-855-428-6074
www.combatmedicalsyste.ms.com

Alphapointe
3611 14th Avenue
Brooklyn, NY 11218 USA
CAGE Code: 056F9

REF 31-115 | CMS-PUB-TMT-04-003
NSN: 6515-01-656-6191
Pat. Info: combatmedicalsyste.ms.com/ip



Made in USA



FDA Registered
Patent Pending

This is a SINGLE USE device.
ISO 9001:2015 Certified

Always store
in one-handed
configuration.





Savior Global
8 Ash Gardens
Hamworthy, Poole, Dorset
BH15 4DE United Kingdom


Limitation of liability: Alphapointe, its employees, agents, contractors, suppliers, and distributors shall assume no liability for injury or damages arising from the application and use of the TMT. ONLY use the TMT as directed in the instructions for use. Do not remove the slider from the strap. The user assumes all risk liability. It is recommended to receive appropriate first aid training.

Standard Use Guidelines: For life threatening hemorrhage situations. For the military in the Care Under Fire situation, treatment normally consists of using a tourniquet immediately to stop major bleeding of the extremities. In field care situation, the trained and authorized rescuer will perform all treatment necessary using the TMT as a last resort and should only be applied when bleeding cannot be stopped and the situation is life threatening.


TWO-HANDED OPERATION INSTRUCTIONS

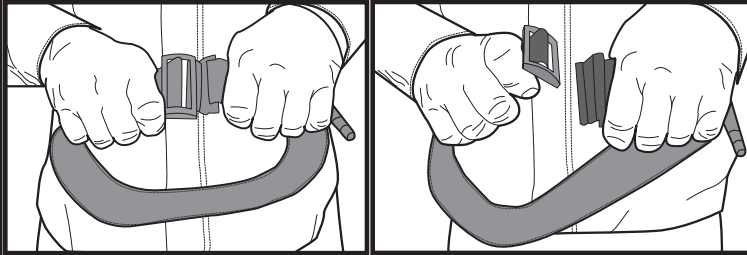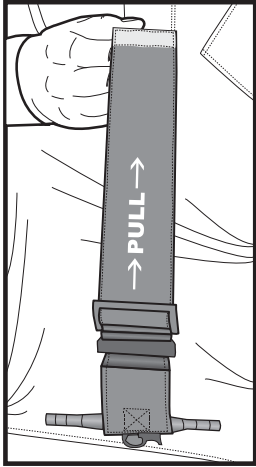



1 Hold the end of the strap by the white time label tab, allow the TMT to fall open. Grab TMT by the buckle and separate the two sections.

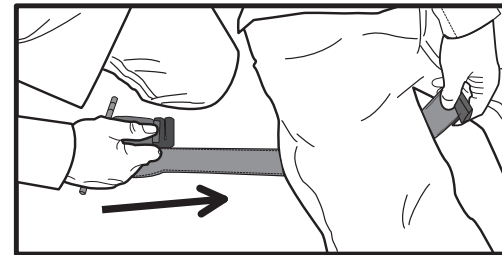

2 Wrap/Feed the TMT around the injured extremity high and tight above the wound, ensuring device is not twisted. Reconnect the buckle.


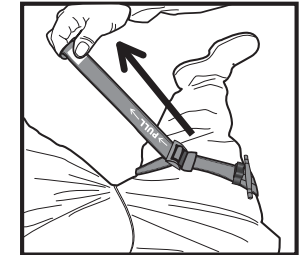


3 Pull time tab until VELCRO® Brand material is separated.




GRIP PULL UP PULL DOWN

4 Grip tail close to the buckle, firmly pull up, out and away from the body and then downward in a quick ratcheting motion. Repeat step until snug around extremity.



ADJUST TWIST

5 Adjust/rotate the TMT on extremity for ease of access to the torsion bar. Twist torsion bar until bleeding stops and the pulse is not present.

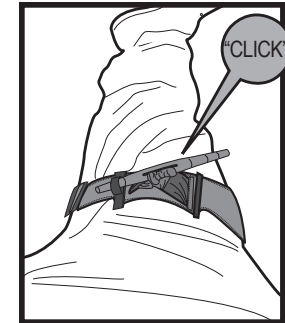

6 Lock the torsion bar into the retainer. Secure excess strap with VELCRO® Brand material.




Distributed by:
 Combat Medical
 5555 Harrisburg Industrial Park Drive
 Harrisburg, NC 28075 USA
 1-855-428-6074
www.combatmedicalsyste.ms.com

Alphapointe
 3611 14th Avenue
 Brooklyn, NY 11218 USA
 CAGE Code: 056F9

REF 31-115 | CMS-PUB-TMT-04-003
 NSN: 6515-01-656-6191
 Pat. Info: combatmedicalsyste.ms.com/ip



Made in USA

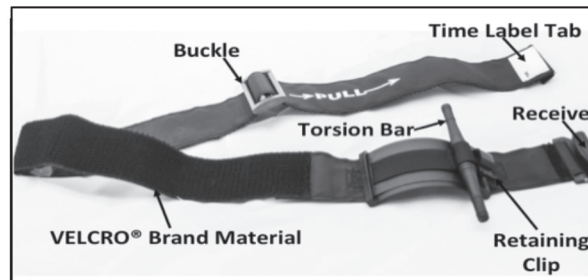

FDA Registered
 Patent Pending

This is a SINGLE USE device
 ISO 9001:2015 Certified

9 Line MEDEVAC Request

- Line 1: Location of the pick-up site
- Line 2: Radio frequency, call sign, and suffix
- Line 3: Number of patients by precedence
- Line 4: Special equipment required
- Line 5: Number of patients
- Line 6: Security at pick-up site
- Line 7: Method of marking pick-up site
- Line 8: Patient nationality and status
- Line 9: NBC Contamination (Peacetime: Terrain)